

KNOW YOUR GLOVE STANDARDS


**TO PROTECT AGAINST
NOVEL CORONAVIRUS
(2019-nCoV)**

“Healthcare workers should wear GLOVES”

- WHO guidance on handling suspected cases of 2019-nCoV [1]



Crucial international standards to ensure adequate protection against 2019-nCoV:

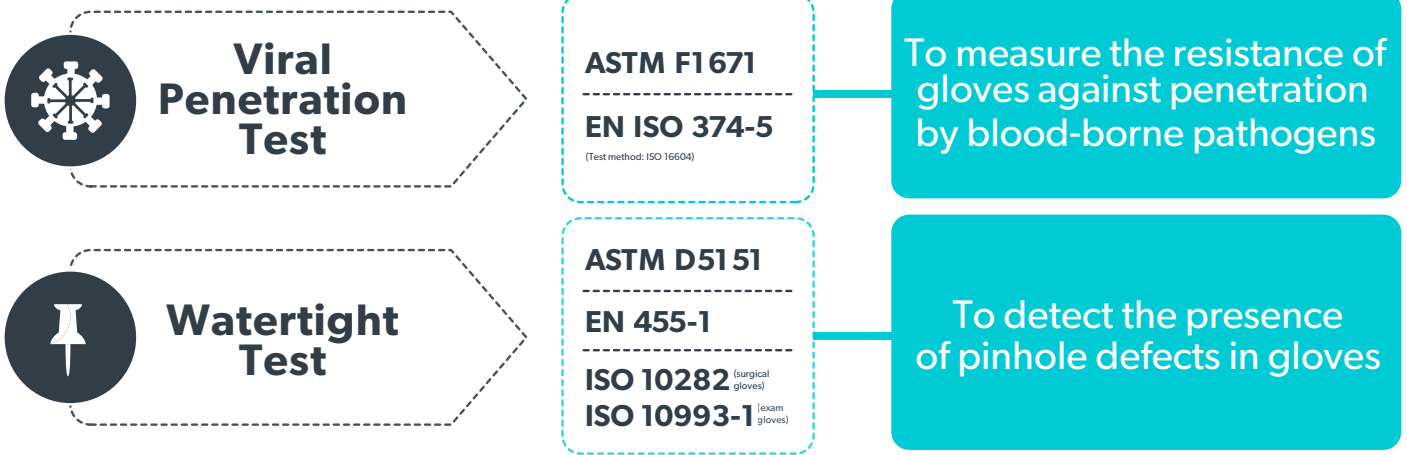

? Does your glove provide **ADEQUATE PROTECTION** against **VIRUSES?**

UNIGLOVES' MEDICAL GLOVES have **PASSED** the above tests*, hence are **SUITABLE** for protection against 2019-nCoV.

Viral Penetration Test	Watertight Test
Our gloves are tested safe against Phi-X174 virus, which is smaller than the 2019-nCoV. Viruses size: Phi-X174 = 25 nm 2019-nCoV = 60-140 nm [2]	We implement stringent control of AQL 0.65 for Stronghold (GM006) gloves and AQL 1.5 for all other nitrile and latex exam gloves.

*Relevant laboratory testing reports are available upon request.

Caution: Proper glove donning and doffing should be observed at all times.

References:

- [https://www.who.int/publications-detail/infection-prevention-and-control-during-health-care-when-novel-coronavirus-\(ncov\)-infection-is-suspected-20200125](https://www.who.int/publications-detail/infection-prevention-and-control-during-health-care-when-novel-coronavirus-(ncov)-infection-is-suspected-20200125)
- https://www.viprbrc.org/brc/home.spg?decorator=corona_ncov

UNIGLOVES UK
Registered in England No: 4010200
VAT registration 791817787

3 Ambley Green, Gillingham Business Park,
Gillingham, ME8 0NJ, UK
+44 (0)800 049 6602
enquiries@unigloves.co.uk
unigloves.co.uk



ughealthcarecorporation.com